

Service Note		
Product	Description:	Service note no.
Finalizer 96K	Upgrade of Finalizer 96K to do Up/Down sampling	720 10 02 07

IMPORTANT:

This note only concerns units with serial no. lower than 1214250.
The upgrade should only be carried out by qualified technicians.

Procedure:

1. Use a PCMCIA card to make a copy of the user presets.
2. Turn Off Power and Disconnect Power Cord.
3. Remove the top lid by loosening five screws, see fig. 1.
4. Remove the old PLL board (P12906-3) by pressing out the lock pins, one in each end, see fig. 2.
5. Install the new PLL board (P12906-5), - check the lock pins locks the board.
6. Mount a 0 ohm resistor at R291, see fig 2.
7. Mount the top lid.
8. Load in application software version 3.5 (or higher)
9. If necessary; load in the user preset. Presets are compatible.

Contents of Up/Down sampling upgrade kit:
PLL circuit board, P12906-5
Service note no. 720 10 02 07

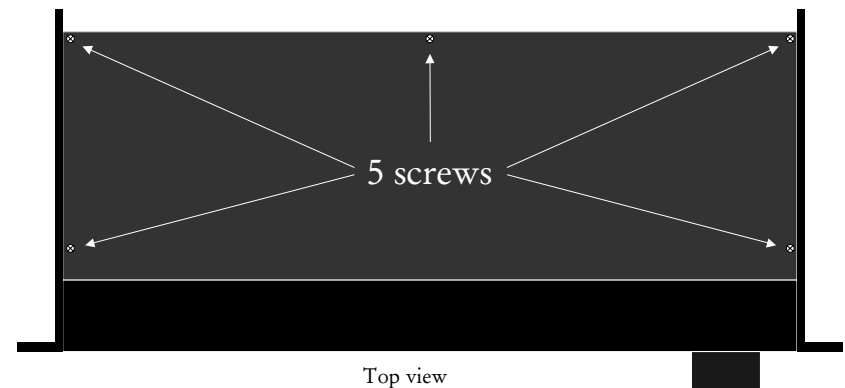


Fig. 1: Screws on top lid

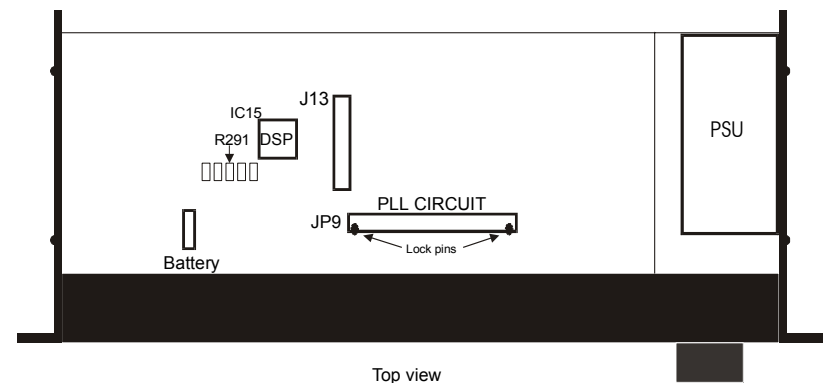


Fig. 2: Location of R291 and PLL circuit board